




HUMELOCKTM REVERSED “SPACER”



DESCRIPTION DU SYSTEME


Once the humeral cut has been done :

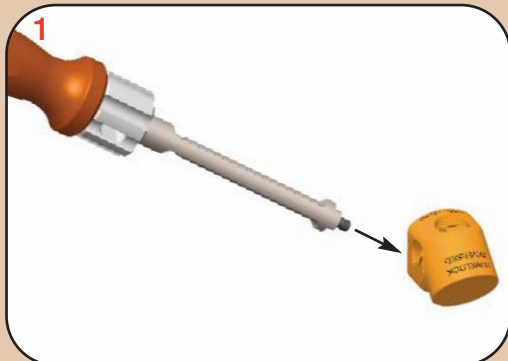

Humelock Reversed spacer assembly :

Screw the guide holder in one of the three threads of the spacer according to the approach :

- left or right deltopectoral
- superior lateral.

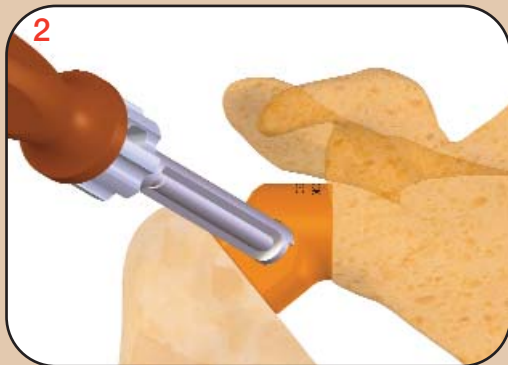


Implementation of the Humelock Reversed spacer :

Put the spacer between the humeral cut and the glenoid by plating the glenoid face of the spacer over the baseplate location.

If the spacer can be introduced, the humeral cut is sufficient to implant a glenosphere $\text{\O}36$ mm and a humeral cup $135/145^\circ +3$ mm (or $+6 / +9$ mm).

Otherwise, a new humeral cut must be done allowing the insertion of the spacer.

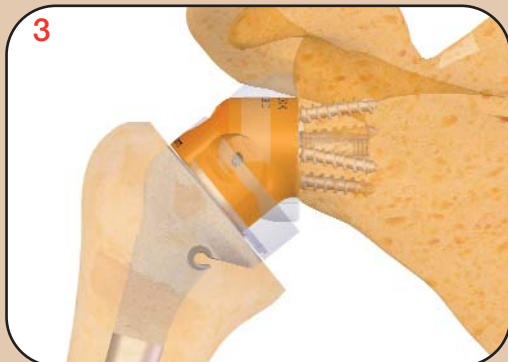

The space used by the spacer corresponds to one humeral cup $135/145^\circ +3$ mm and one glenosphere $\text{\O}36$ mm centered.



1663, rue de Majornas - 01440 Viriat - France
Tél. : (33) 04 74 55 35 55 - Fax : (33) 04 74 52 44 01
E-mail: info@fxsolutions.fr - www.fxsolutions.fr