



ELSEVIER

Contents lists available at ScienceDirect

The Journal of Arthroplasty

journal homepage: www.arthroplastyjournal.org

Primary Arthroplasty

The Effect of Tourniquet Use and Sterile Carbon Dioxide Gas Bone Preparation on Cement Penetration in Primary Total Knee Arthroplasty

Zachary A. Gapinski, BS^a, Elliott J. Yee, BS^a, Kent R. Kraus, BS^a, Evan R. Deckard, BSE^a, R. Michael Meneghini, MD^{a, b, *}^a Department of Orthopaedic Surgery, Indiana University School of Medicine, Indianapolis, IN^b Indiana University Health Physicians, Orthopedics & Sports Medicine, IU Health Hip & Knee Center, Fishers, IN

ARTICLE INFO

Article history:

Received 7 January 2019

Received in revised form

11 March 2019

Accepted 20 March 2019

Available online 28 March 2019

Keywords:

total knee arthroplasty

cement penetration

bone preparation

tourniquet

Radiographic Evaluation System

ABSTRACT

Background: Tourniquetless total knee arthroplasty (TKA) is experiencing resurgence in popularity due to potential pain control benefits. Furthermore, optimal cement technique and implant fixation remain paramount to long-term cemented TKA success, as aseptic loosening continues to be a leading cause of revision. The purpose of this study is to determine how tourniquet use and/or novel bone preparation using sterile, compressed carbon dioxide (CO₂) gas affected cement penetration in TKA.

Methods: A retrospective review was performed on 303 consecutive primary TKAs with the same implant in 3 groups: (1) a tourniquet without sterile CO₂ compressed gas used for bone preparation, (2) no tourniquet with CO₂ gas, and (3) tourniquet use and CO₂ gas bone preparation. Cement penetration was measured on radiographs by two independent, blinded raters across 7 zones defined by the Knee Society Radiographic Evaluation System.

Results: The 3 groups did not differ on age, body mass index, or gender ($P \geq .1$). Cement penetration was greater in 6 of 7 zones with significantly greater cement penetration in 3 zones (tibial anteroposterior zone 2, femoral lateral zones 3A and 3P) in groups that utilized CO₂ gas bone preparation compared to the tourniquet only group ($P \leq .039$).

Conclusion: Bone prepared with CO₂ gas showed significantly more cement penetration in 3 zones with greater cancellous bone. The results suggest that use of CO₂ gas bone preparation may achieve greater cement penetration than using a tourniquet with lavage only.

© 2019 Elsevier Inc. All rights reserved.

Although cemented total knee arthroplasty (TKA) is a widely successful procedure to treat many forms of arthritis, aseptic loosening remains one of the primary causes for early and late revisions [1–5]. Studies and 2017 national registries report that up to 28.7% of all revisions are due to aseptic loosening [3,6–8]. The

One or more of the authors of this paper have disclosed potential or pertinent conflicts of interest, which may include receipt of payment, either direct or indirect, institutional support, or association with an entity in the biomedical field which may be perceived to have potential conflict of interest with this work. For full disclosure statements refer to <https://doi.org/10.1016/j.arth.2019.03.050>.

Source of Funding: The Indiana University Hip and Knee Center Research Program is supported by the Indiana University Health, United States - Indiana University School of Medicine Strategic Research Initiative.

* Reprint requests: R. Michael Meneghini, MD, Department of Orthopaedic Surgery, Indiana University Health Physicians, Indiana University School of Medicine, 13100 136th Street, Suite 2000, Fishers, IN 46037.

<https://doi.org/10.1016/j.arth.2019.03.050>

0883-5403/© 2019 Elsevier Inc. All rights reserved.

projected economic burden of these revisions makes the prevention of TKA failures imperative [9–11]. An evaluation of TKA failures estimated that 40% of early revisions could be avoided, in part, with optimal cement fixation [12]. Increasing the amount of cement into the tibial and femoral bone (cement penetration) has been shown to provide a stronger bone-cement interface which leads to increased stability and long-term survivorship of the implants [13–15].

Traditionally, a tourniquet is used during TKA to optimize cement fixation via minimizing the blood within the cancellous bone to allow more cement penetration and subsequent interdigitation. Studies with and without tourniquet use have reported conflicting results with respect to optimizing cement penetration; however, no difference in implant migration has been reported out to 2 years [16–19]. Furthermore, there are potential clinical drawbacks reported in the literature with using a tourniquet such as increased postoperative blood loss and pain scores with slower

recovery, and decreased quadriceps strength which make tourniquetless TKA appealing [16–18,20–22].

Recently, a novel bone preparation method of sterile, pressurized carbon dioxide (CO₂) gas has been used for its ability to clean out more fluids, fat, and other lipid-soluble debris than a pulsatile lavage alone [23,24]. This technique theoretically offers an even cleaner bone surface for greater bone cement penetration and can be used during TKA to minimize the potential deleterious effect of blood within the cancellous bone during cementation. Recently, the technique of sterile CO₂ compressed gas was utilized in completely tourniquetless TKA, which resulted in less pain and narcotic use in females compared to those utilizing a tourniquet [22]. However, a paucity of published literature exists showing the effect on cement penetration of CO₂ gas as a bone preparation technique. Therefore, the purpose of this study is to evaluate cement penetration in 3 groups: (1) tourniquet only group with no CO₂ gas bone preparation, (2) tourniquet group utilizing CO₂ gas bone preparation, and (3) completely tourniquetless surgery utilizing CO₂ gas used as bone preparation prior to bone cement application in a consecutive series of primary TKAs.

Materials and Methods

With Institutional Review Board approval, a retrospective review of 303 consecutive primary TKAs performed between January 2016 and September 2017 was conducted. All procedures were performed by a single surgeon at one designated hip and knee center. The same perioperative pain and rehabilitation protocols were used for all cases. Of the 303 TKAs, 32 were excluded due to a variety of confounding factors: tibial screw usage (1), prior anterior cruciate ligament surgery (1), patient death within 2 months of surgery unrelated to TKA (2), unable to identify the bone cement used (1), and suboptimal or a lack of 1-month or 1-year radiographs (27) resulting in a sample size of 271 cases.

Radiographic Cement Penetration

All radiographs were accessed in the institution's digital radiographic repository (Synapse, PACS; Fujifilm, Valhalla, NY). Radiographs were obtained by a trained radiologist with a standardized protocol for all cases. Cement penetration was measured according to the zones described by the Knee Society Radiographic Evaluation System (Fig. 1) [25]. Tibial anteroposterior (AP) zones 1 and 2 (Figs. 1 and 2A) represent the medial and lateral inferior surfaces of the tibial baseplate, respectively. Tibial lateral zones 1 and 2 (Figs. 1 and 2B) represent the anterior and posterior distal surfaces of the tibial baseplate, respectively. Femoral lateral zones 3A, 3, and 3P (Figs. 1 and 2B) represent anterior, distal, and posterior proximal surfaces of the femoral component, respectively. For zones 1 and 2 in both the AP and lateral tibial views, cement penetration was measured at the one-third and two-third marks (Fig. 2). For the lateral femoral view, cement penetration in zone 3A was measured at the one-third and two-third mark, while cement penetration in zones 3 and 3P was measured at the one-half mark due to the smaller relative size of these zones to the other zones (Fig. 2B).

Only radiographs with implant views collinear to the X-ray beam were measured to allow the most accurate measurement of cement penetration. Cement penetration measurements were made on 1-month radiographs for all patients unless suboptimal views of the implants were identified. If suboptimal views were found, then the next available postoperative radiograph was used (ie, 1 year, 2 years, etc.). Measurements were collected on digital radiographs with a digital ruler calibrated to the thickness of each tibial baseplate (7.42 mm) which was identical for all sizes of this

particular implant. Once each radiograph was calibrated and each zone was measured horizontally and divided into the appropriate number of sections, the vertical linear distance of cement penetration was measured from the distal-most part of the implant to the distal-most part of the cement mantle (Fig. 2). The cement penetration measurements collected at the one-third and two-third partition of each zone were averaged for an overall cement penetration value for that particular zone.

Measurements were made by 2 independent raters, blinded to the 3 study groups (tourniquet only, CO₂ only, and tourniquet with CO₂). Discrepancies between raters greater than 1.0 mm were resolved by each rater independently revisiting measurements until measurements agreed within 1.0 mm. After discrepancies were resolved, measurements between raters were averaged to calculate an average cement penetration value for each radiographic zone.

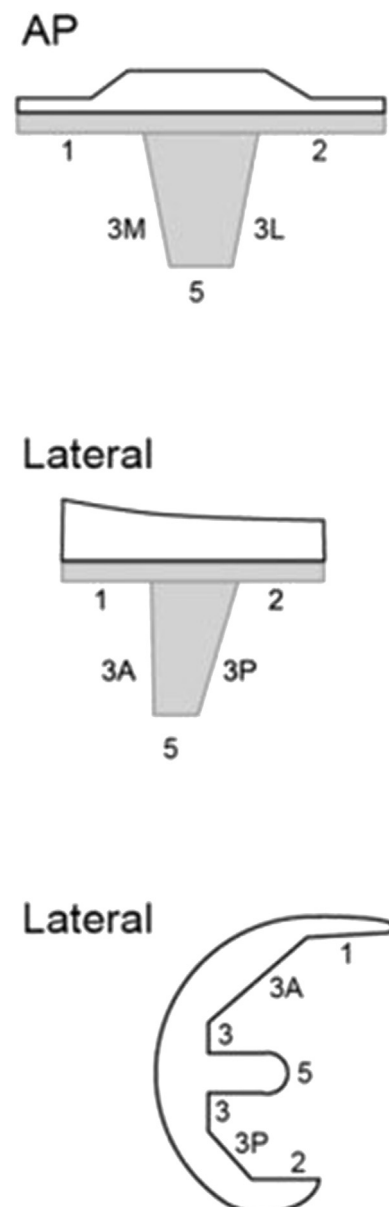


Fig. 1. Radiographic zones defined by the Knee Society Radiographic Evaluation System.

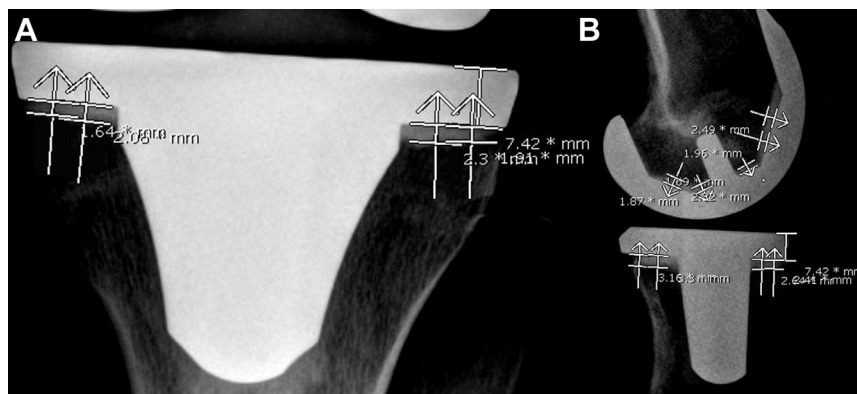


Fig. 2. (A) Cement penetration (AP view). Each AP zone was divided into thirds and cement penetration was measured. (B) Cement penetration (lateral views). Each lateral zone was divided into thirds and measured except for femoral zones 3 and 3P which were divided into half due to the smaller size of these zones. AP, anteroposterior.

Surgical Technique

A median parapatellar approach was used for all procedures. The fat pad was completely excised during all procedures and the patella was subluxed into the lateral gutter without patella eversion in all cases. In addition, a right angle retractor was placed lateral to the tibia retracting the patella clear of the lateral proximal tibia and a retractor placed posteriorly behind the tibia exposing the entire proximal tibial plateau. Standard coronal plane tibial and femoral bone cuts were made with computer-aided navigation (Stryker Navigation, Kalamazoo, MI). One knee arthroplasty system (DJO EMPOWR 3D; DJO Surgical, Austin, TX) was used in all patients and intravenous tranexamic acid was used in all patients. The surgeon routinely utilized a cruciate-retaining implant with a conforming polyethylene insert in all patients with or without preservation of the posterior cruciate ligament. All sclerotic surfaces were prepared with small drill holes to facilitate bone cement interdigitation and were cleaned thoroughly with a pulsatile lavage in all 3 study groups. Medium viscosity polymethylmethacrylate bone cement was mixed with low-dose antibiotics and the components were securely cemented with manual hand pressurization (ie, finger packing) in a standardized manner during the working phase of the bone cement in all cases. The cement was allowed to cure with the knee held in extension and visual confirmation of secured component fixation was obtained. Upon drying, all extraneous cement was removed from all aspects of the knee. Finally, the knee was vigorously irrigated again with a pulsatile lavage to remove any cement particles and the final polyethylene insert was inserted and impacted into a locked position. The only alterations to this protocol were when compressed CO₂ gas (CarboJet; Kinamed, Inc, Camarillo, CA) was used for bone preparation prior to applying the bone cement or a tourniquet was not used. When a tourniquet was not utilized, it is important to clarify that the tourniquet was not applied to the operative leg and therefore not utilized at any point during the procedure, not even during cementation.

The “tourniquet only” group utilized a tourniquet without compressed CO₂ gas for bone preparation. The “CO₂ only” group did not use a tourniquet and used compressed CO₂ gas for bone preparation. The “tourniquet with CO₂” group utilized both a tourniquet and CO₂ gas for bone preparation. All 3 groups received pulsatile lavage regardless of CO₂ gas bone preparation or tourniquet use. All other events for the surgical protocol were unchanged for all cases.

Statistical Analysis

Minitab 17 (State College, PA) was used for statistical analyses. Outliers were assessed with a form of Dixon's outlier test

dependent on the sample size. Data were evaluated for normality using Anderson-Darling tests. Tibial AP zone 1, tibial AP zone 2, tibial lateral zone 1, tibial lateral zone 2, and the overall cement penetration across all 7 zones were normally distributed ($P \geq .456$). Consequently, cement penetration measurements for these five variables were evaluated with an analysis of variance (F), while the cement penetration measurements of the other 3 zones were non-normally distributed ($P \leq .043$) and therefore required a Kruskal-Wallis (H) test adjusted for ties. Pearson's chi-squared (χ^2) test was used to test independence among categorical variables, with Fisher's exact test P values reported for 2×2 contingency tables. A significance level of 0.05 was used for all statistical analyses.

Results

Demographics

Two hundred seventy-one TKAs were available for analysis. Overall, mean age was 67.8 years (standard deviation [SD] 8.7) and median body mass index was 33.0 kg/m². Seventy-two percent ($n = 194$) of the study population was female. TKAs were then grouped by intraoperative tourniquet use and bone preparation method. Thirty-seven percent of the cohort used a tourniquet only with no CO₂ bone preparation ($n = 101$), 34% used a tourniquet and CO₂ bone preparation ($n = 91$), and 29% used CO₂ bone preparation with no tourniquet ($n = 79$). No difference in age, body mass index, or proportion of females to males was detected in the 3 groups (Table 1; $P \geq .1$).

Cement Penetration

The depth of cement penetration was compared in each radiographic zone among the 3 groups. No differences in cement penetration were found for tibial AP zone 1, tibial lateral zone 1, tibial lateral zone 2, or femoral lateral zone 3 (Table 2; $P \geq .173$). However, tibial AP zone 2, femoral lateral zone 3A, and femoral lateral zone 3P showed significantly more cement penetration for groups using the compressed CO₂ gas for bone preparation (Table 2; $P \leq .039$). In fact, one of the 2 groups that utilized the compressed CO₂ gas almost always showed equivalent or greater cement penetration compared to the tourniquet only group (except for tibial lateral zone 2) although some zones did not achieve statistical significance (Fig. 3). The average cement penetration across all 7 zones also showed no difference ($F = 1.12$, $P = .326$); however, the tourniquet with CO₂ gas had the greatest overall cement penetration (2.23 mm, SD 0.41) followed by the CO₂ only group (2.18 mm,

Table 1
Study Group Demographics.

	Tourniquet Only	CO ₂ Only	Tourniquet With CO ₂	Test Statistic	P Value
n (%)	101 (37%)	79 (29%)	91 (34%)	–	–
Mean age (y)	68.9 (SD 8.5)	66.9 (SD 7.9)	67.4 (SD 9.7)	F = 1.35	.261
Median BMI (kg/m ²)	31.0	35.0	33.6	H = 2.56	.279
Female (%)	79%	67%	67%	χ ² = 4.598	.100

ANOVA, analysis of variance; BMI, body mass index; CO₂, carbon dioxide; F, ANOVA test statistic; H, Kruskal-Wallis test statistic; n, sample size; SD, standard deviation; χ², Pearson's chi-squared.

SD 0.50) and then the tourniquet only group (2.13 mm, SD 0.48; Fig. 3).

Discussion

Previous reports have advocated for tourniquet use to enhance cement fixation strength so that blood does not interfere with the bone-cement interface and therefore provides an increased shear strength for the interface [16,26]. However, the use of a tourniquet has been reported to be correlated with potential clinical drawbacks such as higher *postoperative* pain and blood loss, and slower recovery [16,20,22]. Due to these findings, tourniquetless TKAs have experienced a resurgence with similar clinical results compared to tourniquet TKAs [19,27]. In addition, alternative techniques (ie, compressed, sterile CO₂ gas) are being pursued to increase cement penetration and provide increased initial stability and hopefully better long-term survivorship for cemented TKAs.

Cement penetration appears to be a pertinent measure of implant fixation both in the short-term, but also in the longer term as a predictor of TKA longevity. Miller et al [14] conducted a post-mortem retrieval study of 14 TKAs implanted from 0 to 20 years and documented decreasing depth of interdigitation and cement interlock correlated with time in situ. In a subsequent analysis, the authors further loaded retrieved implants in mechanical compression to assess micromotion [28]. The authors demonstrated that TKA tibial implants with less initial interdigitation between cement and bone and more time in service had less current cement-bone interdigitation ($r^2 = 0.86$, $P = .0002$) and tibial

implants with greater initial interdigitation also had less micromotion after in vivo service ($r^2 = 0.36$, $P = .0062$) [28]. This provides direct evidence that greater initial interlock between cement and bone in tibial components of TKA results in more stable constructs with less micromotion with in vivo service and validates utilizing cement penetration as a surrogate for implant fixation and longevity.

Three radiographic zones (tibial AP zone 2, femoral lateral zone 3A, and femoral lateral zone 3P) showed significantly more cement penetration for one of the 2 groups that utilized the CO₂ gas for bone preparation compared to tourniquet alone. These 3 zones tend to have less bone density and greater porosity of cancellous bone, as opposed to the frequently sclerotic medial tibial plateau in osteoarthritic varus knees, and therefore by using the CO₂ gas as a bone preparation technique, cleared out more fat and debris to allow for enhanced cement penetration. Our data corroborate the few studies evaluating the efficacy of CO₂ gas as an effective alternative to other irrigation and lavage techniques [23,24,29,30]. In a cadaver study conducted by Boontanapibul et al [29], cement penetration was measured with calipers and shown to be greater in areas of cancellous bone on the proximal tibia for the group that used the pressurized CO₂ gas for bone preparation compared to pulsatile lavage alone (1.90 vs 1.21 mm, $P = .04$). Similarly, we report significantly greater cement penetration on the proximal tibia with the use of CO₂ gas used for bone preparation compared to pulsatile lavage alone (Fig. 3; 2.08 vs 2.43 mm, $P = .007$). In another cadaveric study, Ravenscroft et al [30] investigated the push out strength of bone cement plugs between bone preparation

Table 2
Cement Penetration (in mm) by Radiographic Zone.

	Tourniquet Only (n = 101)	CO ₂ Only (n = 79)	Tourniquet With CO ₂ (n = 90) ^a	Test Statistic	P Value
Overall					
Average across 7 zones	2.13	2.18	2.23	F = 1.12	.326
Range (min, max)	1.18 3.68	1.02 3.44	1.20 3.45		
AP tibia	n = 69	n = 45	n = 48		
Zone 1	1.79	1.72	1.93	F = 1.01	.367
Range (min, max)	0.26 3.32	0.35 3.00	0.54 4.14		
Zone 2	2.08 ^A	2.34 ^{AB}	2.43 ^B	F = 5.15	.007
Range (min, max)	0.44 3.52	1.03 3.82	1.39 3.98		
Lateral tibia	n = 81	n = 57	n = 64		
Zone 1	2.64	2.72	2.81	F = 0.89	.412
Range (min, max)	1.16 4.35	0.50 4.60	1.08 5.46		
Zone 2	2.61	2.60	2.38	H = 3.50	.173
Range (min, max)	1.12 4.08	1.50 4.54	0.85 4.99		
Lateral femur	n = 75	n = 58	n = 67		
Zone 3A	2.16 ^A	2.48 ^B	2.38 ^{AB}	H = 6.77	.034
Range (min, max)	0.00 3.44	1.26 3.65	1.10 3.57		
Zone 3	1.71	1.76	1.79	H = 0.38	.829
Range (min, max)	0.00 3.19	0.67 3.89	1.02 2.47		
Zone 3P	1.64 ^A	1.90 ^{AB}	1.87 ^B	H = 6.50	.039
Range (min, max)	0.00 2.90	0.00 3.54	0.00 2.93	–	–

Means or medians that do not share a letter are statistically different.

Bold P-values indicate statistical significance at $P < .05$.

F, ANOVA test statistic; CO₂, carbon dioxide; ANOVA, analysis of variance; H, Kruskal-Wallis test statistic; n, sample size; SD, standard deviation; AP, anteroposterior.

^a One significant outlier was removed from the overall cement penetration average (value = 5.22 mm, $r_{22} = 0.54$, $P < .001$).

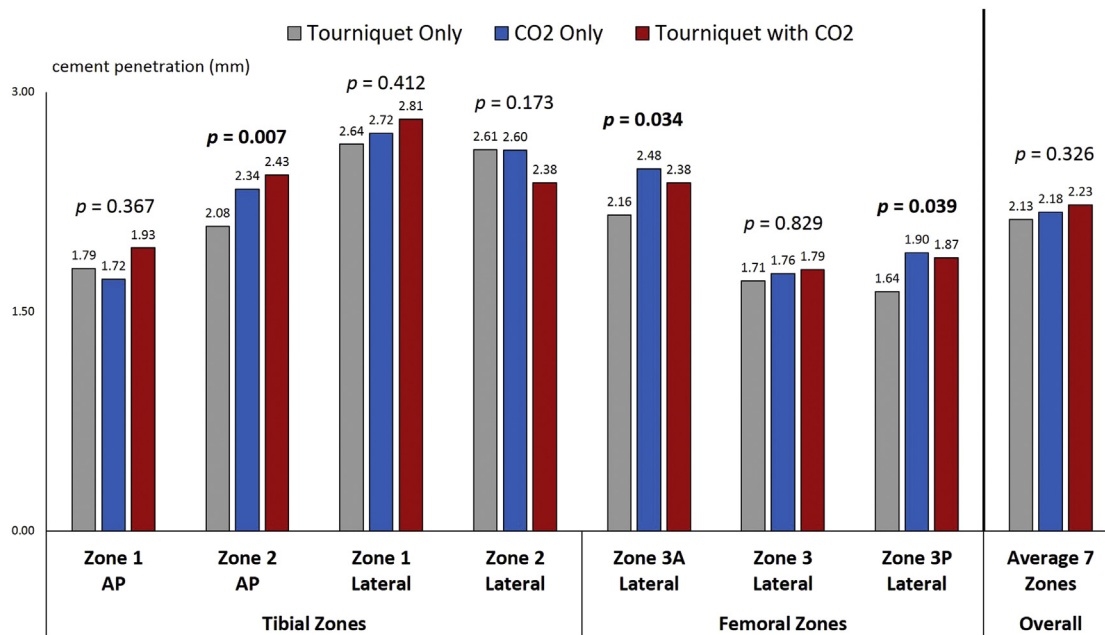


Fig. 3. Cement penetration for all radiographic zones. CO₂ only or tourniquet with CO₂ groups had equivalent or greater penetration compared to tourniquet only in each zone except for tibial lateral zone 2.

techniques of CO₂ compressed gas and standard syringed saline. The authors reported that the required force to remove a bone cement plug was significantly higher when CO₂ gas was used for bone preparation compared to standard saline alone (median force 580.6 vs 366.6 N, $P = .009$) suggesting that the pressurized CO₂ gas provided enhanced bone cement interdigitation and a stronger bone-cement interface [30]. In two other studies, investigating the efficacy of compressed CO₂ gas and osteochondral allografts, both studies found that the use of compressed CO₂ gas more effectively cleared out bone marrow elements than using saline solution only [23,24].

Cement penetration differences were only seen in one of the 2 CO₂ gas groups (with and without a tourniquet) compared to tourniquet with lavage alone. However, considering the potential drawbacks of tourniquet use reported in the literature [16,20–22,31], this may obviate the need for a tourniquet clinically. Therefore, based on the cement penetration data presented here, the use of CO₂ gas without a tourniquet for bone preparation may achieve equivalent cement penetration without the potential drawbacks of tourniquet use [16,20–22,31].

This study had limitations. One limitation was the amount of missing data due to suboptimal radiograph quality with implants not being collinear to the radiograph machine collimator for accurate cement penetration measurements. This strict inclusion criterion also can be a strength to the study as only the most accurate measurements of cement penetration were collected, avoiding erroneous data points. Another limitation was the lack of bone density data, as this metric was not able to be measured with the available tools at our institution, nor is it practical or within the scope of this clinical study. Studies have shown that patients with lower bone density can achieve greater cement penetration and therefore improved initial implant stability [15,32]. Although we did not have access to bone density data for each patient, we do not believe that it was responsible for the difference in cement penetration between the groups. The 3 groups did not differ in the proportion of females to males in any group ($P \geq .1$) or the overall cement penetration between females and males (mean female = 2.16 mm [SD 0.46] and male = 2.21 mm [SD 0.48], $t = 0.78$,

$P = .436$). Finally, a limitation to this study was the slight increase in cost associated with using this device (\$130 USD per case); however, the benefit to using this device could help reduce aseptic loosening rates in TKA and therefore reduce cost in the long term by minimizing costly revisions.

To the authors' knowledge, this is one of the first studies to evaluate in vivo differences in cement penetration using this novel bone preparation method of sterile, pressurized CO₂ gas. These results suggest that a movement toward CO₂ gas bone preparation in cemented TKA could achieve improved implant fixation via greater cement penetration than using a tourniquet with lavage only. The improved cement penetration when using CO₂ gas for bone preparation may lead to less implant loosening and therefore better patient outcomes. Longer follow-up of these cases is recommended to evaluate any differences with implant survivorship related to aseptic loosening.

References

- [1] Schroer WC, Berend KR, Lombardi AV, Barnes CL, Bolognesi MP, Berend ME, et al. Why are total knees failing today? Etiology of total knee revision in 2010 and 2011. *J Arthroplasty* 2013;28:116–9.
- [2] Dyrhovden GS, Lygre SHL, Badawy M, Gothesen O, Furnes O. Have the causes of revision for total and unicompartmental knee arthroplasties changed during the past two decades? *Clin Orthop Relat Res* 2017;475:1874–86.
- [3] Thiele K, Perka C, Matziolis G, Mayr HO, Sostheim M, Hube R. Current failure mechanisms after knee arthroplasty have changed: polyethylene wear is less common in revision surgery. *J Bone Joint Surg Am* 2015;97:715–20.
- [4] Sharkey PF, Hozack WJ, Rothman RH, Shastri S, Jacoby SM. Why are total knee arthroplasties failing today? *Clin Orthop Relat Res* 2002;404:7–13.
- [5] Sharkey PF, Lichstein PM, Shen C, Tokarski AT, Parvizi J. Why are total knee arthroplasties failing today—has anything changed after 10 years? *J Arthroplasty* 2014;29:1774–8.
- [6] American joint replacement registry annual report 2017. Rosemont, IL: American Joint Replacement Registry (AJRR); 2017. <https://www.ajrr.net/publications-data>.
- [7] Australian national joint replacement registry—hip, knee & shoulder arthroplasty annual report 2017. Adelaide, Australia: Australian Orthopaedic Association National Joint Replacement Registry; 2017. <https://aoanjrr.sahmri.com/annual-reports-2017>.
- [8] Canadian joint replacement registry update 2017. Ottawa, Canada: Canadian Institute of Health Information; 2017. <https://www.cihi.ca/sites/default/files/document/cjrr-update-summer-2017-en.pdf>.

- [9] Bozic KJ, Kurtz SM, Lau E, Ong K, Chiu V, Vail TP, et al. The epidemiology of revision total knee arthroplasty in the United States. *Clin Orthop Relat Res* 2010;468:45–51.
- [10] Kurtz S, Ong K, Lau E, Mowat F, Halpern M. Projections of primary and revision hip and knee arthroplasty in the United States from 2005 to 2030. *J Bone Joint Surg Am* 2007;89:780–5.
- [11] Weinstein AM, Rome BN, Reichmann WM, Collins JE, Burbine SA, Thornhill TS, et al. Estimating the burden of total knee replacement in the United States. *J Bone Joint Surg Am* 2013;95:385–92.
- [12] Fehring TK, Odum S, Griffin WL, Mason JB, Nadaud M. Early failures in total knee arthroplasty. *Clin Orthop Relat Res* 2001;392:315–8.
- [13] Macdonald W, Swarts E, Beaver R. Penetration and shear-strength of cement bone interfaces in vivo. *Clin Orthop Relat Res* 1993;286:283–8.
- [14] Miller MA, Goodheart JR, Izant TH, Rimnac CM, Cleary RJ, Mann KA. Loss of cement–bone interlock in retrieved tibial components from total knee arthroplasties. *Clin Orthop Relat Res* 2014;472:304–13.
- [15] Nagel K, Bishop NE, Schlegel UJ, Puschel K, Morlock MM. The influence of cement morphology parameters on the strength of the cement–bone interface in tibial tray fixation. *J Arthroplasty* 2017;32:563–569.e561.
- [16] Pfitzner T, von Roth P, Voerkelius N, Mayr H, Perka C, Hube R. Influence of the tourniquet on tibial cement mantle thickness in primary total knee arthroplasty. *Knee Surg Sports Traumatol Arthrosc* 2016;24:96–101.
- [17] Zhou K, Ling T, Wang H, Zhou Z, Shen B, Yang J, et al. Influence of tourniquet use in primary total knee arthroplasty with drainage: a prospective randomised controlled trial. *J Orthop Surg Res* 2017;12:172.
- [18] Jawhar A, Stetzelberger V, Kollowa K, Obertacke U. Tourniquet application does not affect the periprosthetic bone cement penetration in total knee arthroplasty. *Knee Surg Sports Traumatol Arthrosc* 2018. <https://doi.org/10.1007/s00167-018-5330-7>. [Epub ahead of print].
- [19] Ejaz A, Laursen AC, Jakobsen T, Rasmussen S, Nielsen PT, Laursen MB. Absence of a tourniquet does not affect fixation of cemented TKA: a randomized RSA study of 70 patients. *J Arthroplasty* 2015;30:2128–32.
- [20] Ejaz A, Laursen AC, Kappel A, Laursen MB, Jakobsen T, Rasmussen S, et al. Faster recovery without the use of a tourniquet in total knee arthroplasty. *Acta Orthop* 2014;85:422–6.
- [21] Dennis DA, Kittelson AJ, Yang CC, Miner TM, Kim RH, Stevens-Lapsley JE. Does tourniquet use in TKA affect recovery of lower extremity strength and function? A randomized trial. *Clin Orthop Relat Res* 2016;474:69–77.
- [22] Kheir MM, Ziemba-Davis M, Dilley JE, Hood Jr MJ, Meneghini RM. Tourniquetless total knee arthroplasty with modern perioperative protocols decreases pain and opioid consumption in women. *J Arthroplasty* 2018;33:3455–9.
- [23] Baumann CA, Baumann JR, Bozynski CC, Stoker AM, Stannard JP, Cook JL. Comparison of techniques for preimplantation treatment of osteochondral allograft bone. *J Knee Surg* 2019;32:97–104.
- [24] Meyer MA, McCarthy MA, Gitelis ME, Poland SG, Urita A, Chubinskaya S, et al. Effectiveness of lavage techniques in removing immunogenic elements from osteochondral allografts. *Cartilage* 2017;8:369–73.
- [25] Meneghini RM, Mont MA, Backstein DB, Bourne RB, Dennis DA, Scuderi GR. Development of a modern knee society radiographic evaluation system and methodology for total knee arthroplasty. *J Arthroplasty* 2015;30:2311–4.
- [26] Majkowski RS, Bannister GC, Miles AW. The effect of bleeding on the cement–bone interface—an experimental–study. *Clin Orthop Relat Res* 1994;299:293–7.
- [27] Molt M, Harsten A, Toksvig-Larsen S. The effect of tourniquet use on fixation quality in cemented total knee arthroplasty a prospective randomized clinical controlled RSA trial. *Knee* 2014;21:396–401.
- [28] Miller MA, Terbush MJ, Goodheart JR, Izant TH, Mann KA. Increased initial cement–bone interlock correlates with reduced total knee arthroplasty micromotion following in vivo service. *J Biomech* 2014;47:2460–6.
- [29] Boontanapibul K, Ruangsomboon P, Charoencholvanich K, Pornrattanamaneewong C. Effectiveness testing of combined innovative pressurized carbon dioxide lavage and pulsatile normal saline irrigation to enhance bone cement penetration in total knee replacement: a cadaveric study. *J Med Assoc Thai* 2016;99:1198–202.
- [30] Ravenscroft MJ, Charalambous CP, Mills SP, Woodruff MJ, Stanley JK. Bone–cement interface strength in distal radii using two medullary canal preparation techniques: carbon dioxide jet cleaning versus syringed saline. *Hand Surg* 2010;15:95–8.
- [31] Abdel-Salam A, Eyres KS. Effects of tourniquet during total knee arthroplasty. A prospective randomised study. *J Bone Joint Surg Br* 1995;77:250–3.
- [32] Graham J, Ries M, Pruitt L. Effect of bone porosity on the mechanical integrity of the bone–cement interface. *J Bone Joint Surg Am* 2003;85A:1901–8.