





## XPERT WRIST 2.4 UPDATE HOW TO RESTORE BONE ANATOMY?

### OSTEOTOMY PLATE

Dedicated plates and instruments allowing to manage ulnar variance

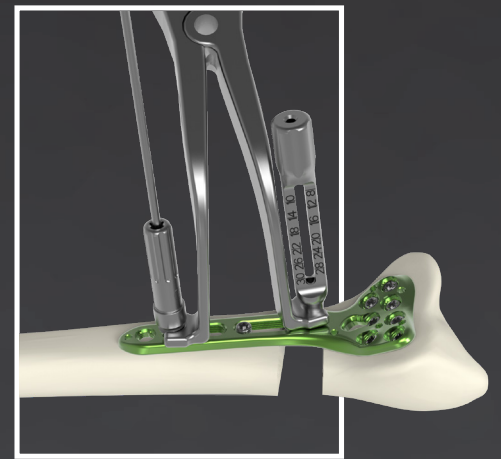

- Precontoured implant
- 2 oblong locking holes allowing up to 10 mm of distraction
- Dedicated distractor

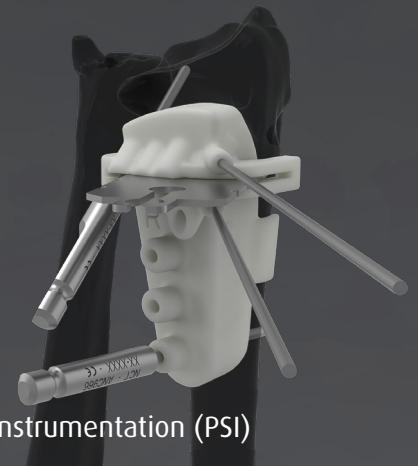

Compatible with the Xpert Wrist 2.4 system and with our Patient Specific Instrumentation (PSI)

Medical device class IIb - CE1639 SGS BE - Read labeling before use. Non-contractual pictures.

**NEWCLIP TECHNICS**  
 PA de la Lande Saint Martin  
 45 rue des Garottières  
 44115 Haute-Goulaine, France  
 +33 (0)2 28 21 23 25  
 orders@newcliptechnics.com  
 www.newcliptechnics.com

**NEWCLIP TECHNICS USA**  
 Newclip USA  
 642 Larkfield Center  
 Santa Rosa CA 95403, USA  
 +1 707 230 5078  
 customerservice@newclipusa.com  
 www.newclipusa.com

**NEWCLIP TECHNICS GERMANY**  
 Newclip GmbH  
 Pröllstraße 11  
 D-86157 Augsburg, Deutschland  
 +49 (0)821 650 749 40  
 info@newclipgmbh.com  
 www.newclipgmbh.de

**NEWCLIP TECHNICS JAPAN**  
 Newclip Technics Japan K.K.  
 KKK Bldg. 502, 3-18-1 Asakusabashi  
 Taito-Ku, Tokyo, 111-0053, Japan  
 +81 (0)3 58 25 49 81  
 Fax: +81 (0)3 58 25 49 86  
 www.newcliptechnics.com

**NEWCLIP TECHNICS AUSTRALIA**  
 Newclip Australia  
 3B/11 Donkin Street  
 West End 4101, Australia  
 +61 (0)2 81 886 110  
 solutions@newclipaustralia.com  
 www.newcliptechnics.com